

Спектрофотометр UV-Vis Ultrospec 7500

Технические характеристики

По вопросам продаж и поддержки обращайтесь:

Алматы (727)345-47-04
Ангарск (3955)60-70-56
Архангельск (8182)63-90-72
Астрахань (8512)99-46-04
Барнаул (3852)73-04-60
Белгород (4722)40-23-64
Благовещенск (4162)22-76-07
Брянск (4832)59-03-52
Владивосток (423)249-28-31
Владикавказ (8672)28-90-48
Владимир (4922)49-43-18
Волгоград (844)278-03-48
Вологда (8172)26-41-59
Воронеж (473)204-51-73
Екатеринбург (343)384-55-89

Иваново (4932)77-34-06
Ижевск (3412)26-03-58
Иркутск (395)279-98-46
Казань (843)206-01-48
Калининград (4012)72-03-81
Калуга (4842)92-23-67
Кемерово (3842)65-04-62
Киров (8332)68-02-04
Коломна (4966)23-41-49
Кострома (4942)77-07-48
Краснодар (861)203-40-90
Красноярск (391)204-63-61
Курск (4712)77-13-04
Курган (3522)50-90-47
Липецк (4742)52-20-81

Магнитогорск (3519)55-03-13
Москва (495)268-04-70
Мурманск (8152)59-64-93
Набережные Челны (8552)20-53-41
Нижний Новгород (831)429-08-12
Новокузнецк (3843)20-46-81
Ноябрьск (3496)41-32-12
Новосибирск (383)227-86-73
Омск (3812)21-46-40
Орел (4862)44-53-42
Оренбург (3532)37-68-04
Пенза (8412)22-31-16
Петрозаводск (8142)55-98-37
Псков (8112)59-10-37
Пермь (342)205-81-47

Ростов-на-Дону (863)308-18-15
Рязань (4912)46-61-64
Самара (846)206-03-16
Санкт-Петербург (812)309-46-40
Саратов (845)249-38-78
Севастополь (8692)22-31-93
Саранск (8342)22-96-24
Симферополь (3652)67-13-56
Смоленск (4812)29-41-54
Сочи (862)225-72-31
Ставрополь (8652)20-65-13
Сургут (3462)77-98-35
Сыктывкар (8212)25-95-17
Тамбов (4752)50-40-97
Тверь (4822)63-31-35

Тольятти (8482)63-91-07
Томск (3822)98-41-53
Тула (4872)33-79-87
Тюмень (3452)66-21-18
Ульяновск (8422)24-23-59
Улан-Удэ (3012)59-97-51
Уфа (347)229-48-12
Хабаровск (4212)92-98-04
Чебоксары (8352)28-53-07
Челябинск (351)202-03-61
Череповец (8202)49-02-64
Чита (3022)38-34-83
Якутск (4112)23-90-97
Ярославль (4852)69-52-93

Россия +7(495)268-04-70

Казахстан +7(727)345-47-04

Беларусь +(375)257-127-884

Узбекистан +998(71)205-18-59

Киргизия +996(312)96-26-47

эл.почта: bmq@nt-rt.ru || сайт: <https://biochrom.nt-rt.ru/>



Ultrospec 7500 UV-Vis Spectrophotometer

Simple to use and with all the features you need, the Ultrospec 7500 spectrophotometer is perfect for any manufacturing or production laboratory. It's reliable, robust, and one of the most precise quality control instruments on the market.

Precise, with consistent results

Your work depends on accurate, consistent results – and the Ultrospec 7500 delivers. With a <math><2\text{nm}</math> spectral bandwidth and wavelength accuracy of $\pm 1\text{ nm}</math>, it offers a high degree of precision and reproducibility. Never doubt your data again.$

Powerful onboard firmware that saves you time

The onboard firmware provides a wide selection of pre-loaded methods – including applications for quantification of nucleic acids, proteins, and cell density – as well as a menu of commonly available fluorescent dyes for your highest-precision requirements.

8-Cell sample carousel as standard

Need to run multiple samples at once? The Ultrospec 7500 includes an automated 8-cell sample carousel, making it easy to increase your throughput (and finish faster).

GLP-compliant

The easy-to-activate GLP mode ensures that your data adheres to Good Laboratory Practice requirements. Documentation–flexible test templates validate certified calibration standards, and the automated data log stores performance history.

Energy-efficient touchscreen display.

The system includes an intuitive, easy-to-use, 800×480-pixel backlit color LCD display with touch panel navigation of the instrument’s built-in firmware. When the display is off, the only power consumed is by the touch screen controller. The instrument exits sleep mode with a touch of the screen. Easier on you, and easier on the planet.

Dependable and built to last.

There’s a reason Biochrom is one of the world’s leading spectrophotometry brands: some of our customers have been using the same machine for over 20 years. No planned obsolescence here. Our level of quality, dependability, and customer service is completely unmatched.

IQ/OQ/PQ compliance available

If your lab requires IQ (Installation Qualification), OQ (Operation Qualification), or PQ (Performance Qualification) compliance, your Ultrospec 7500 can be customized to meet your

needs. Contact us to learn more.

21 CFR Part 11-compliant software is also available.

All the accessories (and flexibility) you need.

Looking for one spectrophotometer that does it all? If your lab has unique needs, the optional accessories can help you customize your Ultrospec 7500 to suit them.

- Printers
- Sippers
- Heating
- Various cell accessories
- And more.

TECHNICAL SPECIFICATIONS	
SPECIFICATION	DATA
Wavelength Range	190 to 1100 nm
Monochromator	1200 lines/mm Aberration corrected concave grating
Wavelength Calibration	Automatic upon switch on
Beam Height	15 mm
Spectral Bandwidth	<2 nm
Wavelength Accuracy	±1 nm
Wavelength Reproducibility	±0.5 nm

TECHNICAL SPECIFICATIONS

SPECIFICATION	DATA
Light Sources	Xenon flash lamp
Detector	Two silicon photodiodes
Photometric Range	-3.000 to 3.000 A, 0.1 to 100000 %T
Photometric Accuracy	±0.5 % or ±0.003 A whichever is greater at 546 nm
Photometric Reproducibility	±0.5 % to 3.000 A at 546 nm
Stray Light	<0.05 %T at 220 nm using NaI or at 340 nm using NaNO ₂ , <0.10 %T at 380 using NaNO ₂ ±0.01 A/h at 340 nm
Stability	±0.001 A/h at 340 nm for 0 A
Noise	±0.002 peak to peak ± 0.0005 RMS at 340 nm for 0 A
Digital Output	USB Flash Drive, PC via PVC software, Optional Bluetooth
Data Export	USB Flash Drive: .tsv, native PVC format
Method Storage	156 with PIN number protection
Graphical Display	Yes, zoom and track function
Sample ID	Yes
Languages	English, German, French, Spanish, Italian, Japanese, Chinese
Dimensions	510 × 350 × 160 mm
Weight	13.00 kg
Power Input	19 VDC at max 90 VA from a supplied 100 to 240 V~, 50/60 Hz Mains Power Adapter

^ **Ultrospec 7500**

ITEM #: 80-2140-60

Ultrospec 7500, includes Power Adapter, Sample Cuvettes, Quick Start Guide

Spectrophotometry Essential to your lab—essential to your work



Is your equipment up to spec?


As a scientist involved in high throughput of routine samples, often with different requirements, state-of-the-art spectrophotometry equipment is vital to the success of your work. Whether you are a researcher or a quality control technician working in a pharmaceutical, academic research or industrial manufacturing lab, you depend on accurate, consistent results across multiple samples—every day. This becomes even more critical if you additionally face regulatory burdens, such as GLP, 21 CFR part 11 compliance or IQ/OQ.

In fact, when it comes to quality control in your lab, it can be a daunting challenge to keep up with rapidly changing technologies and regulations. How confident are you that your spectrophotometry equipment is state-of-the-art and compliant, so that you can continuously optimize your quality analysis work?

Count on best-in-class instruments...

Biochrom, an affiliate of Harvard Bioscience, has been delivering best-in-class UV-Vis spectrophotometers for over 40 years to a dedicated global base of thousands of scientists just like you.

Cited tens of thousands of times in research publications since its launch in 1982, our Ultrospec range has been installed in all types of labs across the globe. The newest member of this range, the Ultrospec 7500 UV-Visible spectrophotometer builds on this legacy to give you the highest level of confidence in your spectrophotometric analysis and quality control work for years to come.

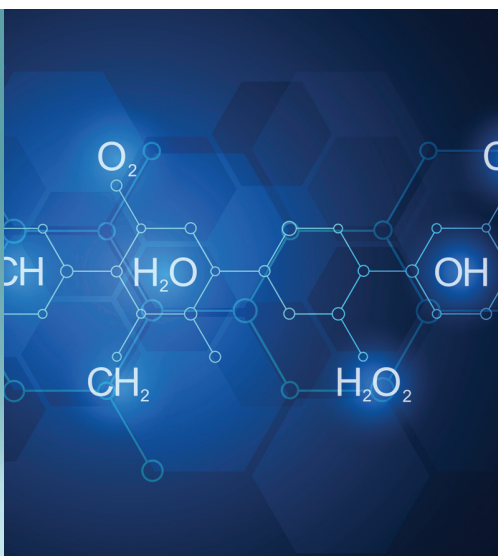

Ultrospec 7500

- **Powerful**—Onboard firmware includes a wide selection of pre-loaded methods
- **Efficient**—Easily transfer results and method information via the USB port using the simple screen capture function
- **Intuitive**—Easy-to-use, icon-driven color touch screen for on-board control and analysis

...backed by superior support services

Your instruments must receive regular verification and meet stringent regulatory requirements, critical for laboratory auditing and quality control.



From initial installation qualification (IQ) to operational qualification (OQ) and ongoing performance qualification (PQ), you can count on Biochrom's expert team to deliver the necessary validation testing required to keep your lab compliant—and running smoothly.

Biochrom deploys the National Institute of Standards and Technology (NIST) traceable standards to demonstrate evidence of quality control according to ISO/IEC 17025.

Ultrospec 7500—Powerful Simplicity



The Ultrospec 7500 is a simple-to-use instrument—with highly advanced performance functionality, and a sophisticated GLP mode to ensure high quality, consistent and reliable results. Versatile and precise, this instrument is ideal for use in any high-end, manufacturing or production laboratory.

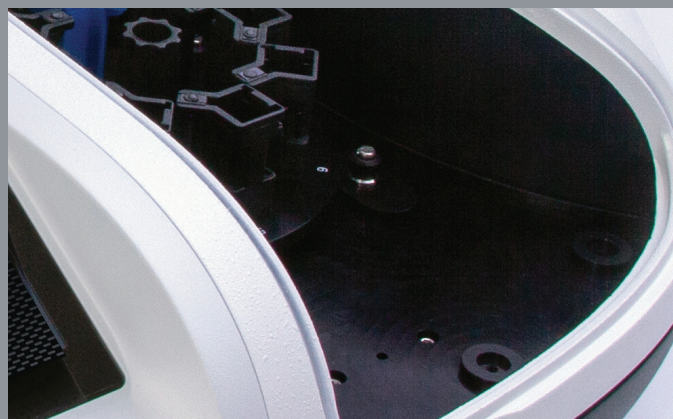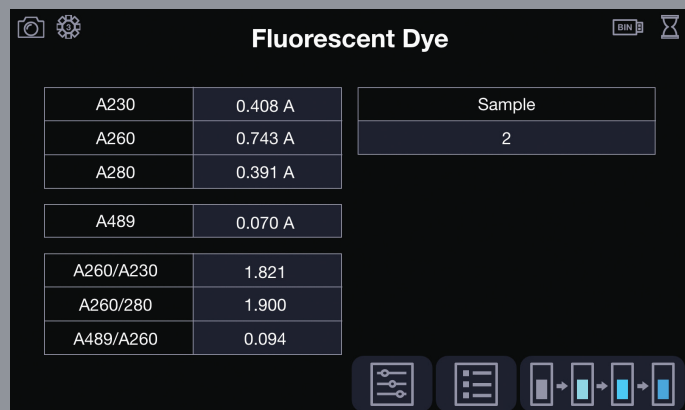

1 Powerful, Onboard Firmware

The onboard firmware provides a wide selection of pre-loaded methods for life sciences, including applications for quantification of nucleic acids, proteins and cell density. Measurements may be taken via direct absorbance, or by accessing the pre-loaded menu of commonly available fluorescent dyes for high precision requirements.

2 Versatile Sampling Options


The Ultrospec 7500 comes with an automated 8-cell sample carousel. It also has a wide range of optional accessories, such as a sippers, heating and various cell accessories, for the ultimate in flexibility.



3 Modern, Energy-Efficient Display


The system has an 800×480-pixel resolution backlit LCD color display with touch panel navigation of the instrument's built-in firmware. When the display is off, the only power consumed is by the touch screen controller. Instrument exits sleep mode with a touch of the screen.

Intuitive Control and Powerful Analysis

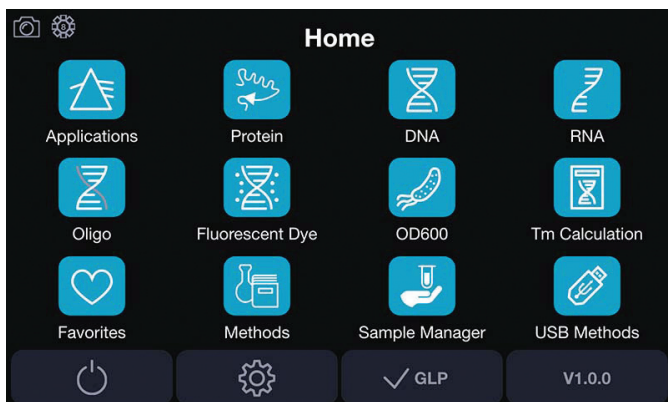

Instrument Homescreen

With quick access to common applications from the homescreen, users are always just a few clicks away from the next set of sample readings.

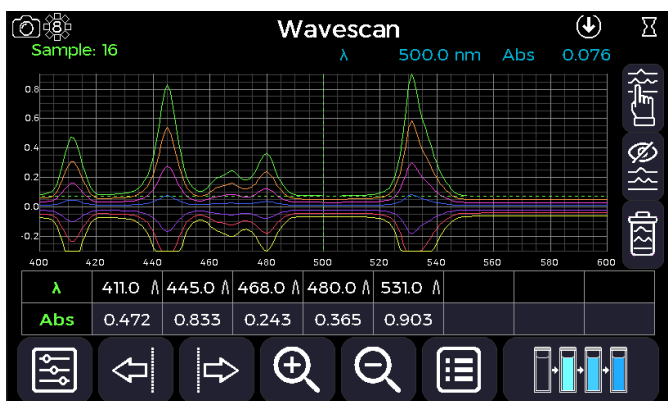

Powerful Onboard Analysis

Color-coded sample overlays allow for quick visual analysis of multiple sample reads, along with zoom and track functionality for more in depth peak analysis.

Ultrospec 7500 IQ/OQ/PQ Services:

- Installation Qualification (IQ)—ensures quality-controlled system installation (location, environment, complete system set-up)
- Operational Qualification (OQ)—validates that system functionality meets manufacturer specifications
- Performance Qualification (PQ)—provides protocols for ongoing validation of your instrument
- Documentation—flexible test templates validate certified calibration standards, robust, automated data log stores performance history
- For on-site IQ/OQ/PQ services specific to your country, please contact your local Biochrom representative

Specifications and Ordering Information

TECHNICAL SPECIFICATIONS	
Wavelength Range	190 to 1100 nm
Monochromator	1200 lines/mm Aberration corrected concave grating
Wavelength Calibration	Automatic upon switch on
Beam Height	15 mm
Spectral Bandwidth	<2 nm
Wavelength Accuracy	±1 nm
Wavelength Reproducibility	±0.5 nm
Light Sources	Xenon flash lamp
Detector	Two silicon photodiodes
Photometric Range	-3.000 to 3.000 A, 0.1 to 100%T
Photometric Accuracy	±0.5 % or ±0.003 A whichever is greater at 546 nm
Photometric Reproducibility	±0.5 % to 3.000 A at 546 nm
Stray Light	<0.05 %T at 220 nm using NaI or at 340 nm using NaNO ₂ , <0.10 %T at 380 using NaNO ₂ ±0.01 A/h at 340 nm
Stability	±0.001 A/h at 340 nm for 0 A
Noise	±0.002 peak to peak ± 0.0005 RMS at 340 nm for 0 A
Digital Output	USB Flash Drive, PC via PVC software, Optional Bluetooth
Data Export	USB Flash Drive: .tsv, native PVC format
Method Storage	156 with PIN number protection
Graphical Display	Yes, zoom and track function
Sample ID	Yes
Languages	English, German, French, Spanish, Italian, Japanese, Chinese
Dimensions	510 × 350 × 160 mm
Weight	13.00 kg
Power Input	19 VDC at max 90 VA from a supplied 100 to 240 V~, 50/60 Hz Mains Power Adapter

ORDERING INFORMATION	
80-2140-60	Ultrospec 7500
80-2140-62	Printer accessory Ultrospec 7500
80-7100-33	Resolution CFR Software
80-2119-89	IQ/OQ Documentation for Ultrospec 7500
80-2119-90	PQ Documentation for Ultrospec 7500

По вопросам продаж и поддержки обращайтесь:

Алматы (727)345-47-04
Ангарск (3955)60-70-56
Архангельск (8182)63-90-72
Астрахань (8512)99-46-04
Барнаул (3852)73-04-60
Белгород (4722)40-23-64
Благовещенск (4162)22-76-07
Брянск (4832)59-03-52
Владивосток (423)249-28-31
Владикавказ (8672)28-90-48
Владимир (4922)49-43-18
Волгоград (844)278-03-48
Вологда (8172)26-41-59
Воронеж (473)204-51-73
Екатеринбург (343)384-55-89

Иваново (4932)77-34-06
Ижевск (3412)26-03-58
Иркутск (395)279-98-46
Казань (843)206-01-48
Калининград (4012)72-03-81
Калуга (4842)92-23-67
Кемерово (3842)65-04-62
Киров (8332)68-02-04
Коломна (4966)23-41-49
Кострома (4942)77-07-48
Краснодар (861)203-40-90
Красноярск (391)204-63-61
Курск (4712)77-13-04
Курган (3522)50-90-47
Липецк (4742)52-20-81

Магнитогорск (3519)55-03-13
Москва (495)268-04-70
Мурманск (8152)59-64-93
Набережные Челны (8552)20-53-41
Нижний Новгород (831)429-08-12
Новокузнецк (3843)20-46-81
Ноябрьск (3496)41-32-12
Новосибирск (383)227-86-73
Омск (3812)21-46-40
Орел (4862)44-53-42
Оренбург (3532)37-68-04
Пенза (8412)22-31-16
Петрозаводск (8142)55-98-37
Псков (8112)59-10-37
Пермь (342)205-81-47

Ростов-на-Дону (863)308-18-15
Рязань (4912)46-61-64
Самара (846)206-03-16
Санкт-Петербург (812)309-46-40
Саратов (845)249-38-78
Севастополь (8692)22-31-93
Саранск (8342)22-96-24
Симферополь (3652)67-13-56
Смоленск (4812)29-41-54
Сочи (862)225-72-31
Ставрополь (8652)20-65-13
Сургут (3462)77-98-35
Сыктывкар (8212)25-95-17
Тамбов (4752)50-40-97
Тверь (4822)63-31-35

Тольятти (8482)63-91-07
Томск (3822)98-41-53
Тула (4872)33-79-87
Тюмень (3452)66-21-18
Ульяновск (8422)24-23-59
Улан-Удэ (3012)59-97-51
Уфа (347)229-48-12
Хабаровск (4212)92-98-04
Чебоксары (8352)28-53-07
Челябинск (351)202-03-61
Череповец (8202)49-02-64
Чита (3022)38-34-83
Якутск (4112)23-90-97
Ярославль (4852)69-52-93

Россия +7(495)268-04-70

Казахстан +7(727)345-47-04

Беларусь +(375)257-127-884

Узбекистан +998(71)205-18-59

Киргизия +996(312)96-26-47

эл.почта: bmq@nt-rt.ru || сайт: <https://biochrom.nt-rt.ru/>